



This is a summary test procedure. Refer to the current Operator's Manual for the complete procedure.

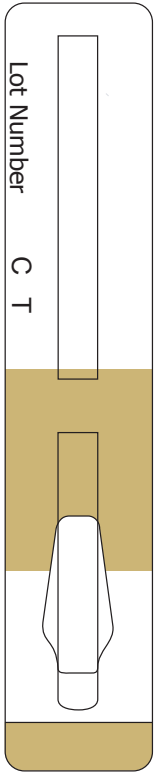


Place completed strip here.

**INVALID**




Re-test INVALID samples.

**POSITIVE**



**NEGATIVE**



**Note:** Visual interpretation is NOT accepted.

**PROCEDURE**

1



Verify incubator temperature is  $56 \pm 1^\circ\text{C}$ .  
Shake milk sample and label test strip.  
Place strip in incubator and use tab to peel tape back to "Peel to here" line.

2



Slowly pipet 300  $\mu\text{l}$  sample into sample compartment at ROSA® Incubator indicator line (as shown).  
Reseal tape over sample compartment.  
Close lid on incubator and tighten latch.  
Incubate for 3 minutes, but not more than 4 minutes.

3



Remove tests from incubator.  
Visually inspect C (control) line for even development.  
Read with ROSA® Reader.  
Insert clean and visually valid test strip in ROSA Reader and read results on MRL channel in 2-line mode (slow-blinking).

Charm Sciences, Inc.  
659 Andover Street, Lawrence, Massachusetts, 01843-1032, USA | [www.charm.com](http://www.charm.com)

© 2012 Charm Sciences, Inc. Charm, ROSA names are registered trademarks, and test strip product packaging is trade dress, of Charm Sciences, Inc. MRK-625-001 0512